



DS Implants™

DS OmniTaper™
Surgical product catalog





All Dentsply Sirona Instructions for Use are available on www.dentsplysirona.com/ifu

All products may not be regulatory cleared/released/licensed in all markets. Please contact the local Dentsply Sirona sales office for current product assortment and availability.

To improve readability for our customers, Dentsply Sirona does not use ® or ™ in body copy. However, Dentsply Sirona does not waive any right to the trademark and nothing herein shall be interpreted to the contrary.

Product illustrations are not to scale.



CONTENTS

1. Implant packaging	4
Color coding	4
2. Implants	5
3. Cover Screw	6
4. TempBase Cap	6
5. Healing abutments	6
6. Instruments	9
Initial drills	9
Drills	9
Taps	10
Implant drivers	11
Planning aids	12
Torque Wrench	13
Driver	13
Surgical Trays	14
Washtray & Overlay	16
Sterilization Container & Reusable Filter	17
7. Guided Surgery Instruments	18
Punch	18
Drills	18
Taps	20
Sleeves	21
Driver	21
Sleeves for Driver	21
Stabilization Abutment	22
Positioning Aid	22
Surgical Trays	22
8. Material specifications	25
9. Index	26

1. Implant packaging

DS OmniTaper implants are supplied in a double-blister package with an outer carton.




Outer box

- Specific color coding, diameter and prominent implant length information on side labels
- Data matrix code on two sides
- Stackable, with all important product information visible
- Instructions For Use (IFU) available electronically (eIFU): ifu.dentsplysirona.com



Outer blister

- Peel-off label with batch code for convenience treatment documentation

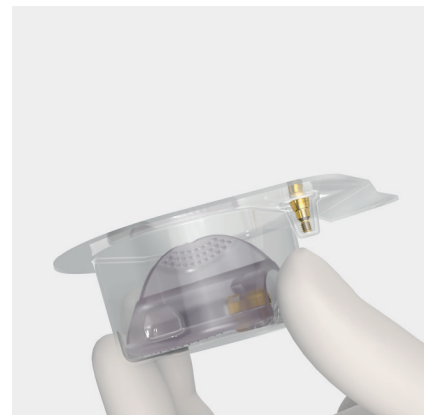

Inner blister

- Inner sterile package
- Implant shuttle with implant and cover screw
- Peel-off label with batch code for convenience treatment documentation

Color coding

The DS OmniTaper implant is available in five diameters and six lengths. The color coding makes it easy to identify the correct connection and to select the right prosthetic components.

Implant Ø	3.0mm	3.4mm	3.8mm	4.5mm	5.5mm
Connections	XS	S	M	L	XL
Lengths	-	-	8mm	8mm	8mm
	-	9.5mm	9.5mm	9.5mm	9.5mm
	11mm	11mm	11mm	11mm	11mm
	13mm	13mm	13mm	13mm	13mm
	15mm	15mm	15mm	15mm	15mm
	-	18mm	18mm	18mm	-

2. Implants

XS OmniTaper EV Ø3.0



Length mm	11	13	15
Order No.	68011140	68011141	68011142

S OmniTaper EV Ø3.4




Length mm	9.5	11	13	15	18
Order No.	68011143	68011144	68011145	68011146	68011147

M OmniTaper EV Ø3.8



Length mm	8	9.5	11	13	15	18
Order No.	68011148	68011149	68011150	68011151	68011152	68011153



L OmniTaper EV Ø4.5



Length mm	8	9.5	11	13	15	18
Order No.	68011154	68011155	68011156	68011157	68011158	68011159

XL OmniTaper EV Ø5.5



Length mm	8	9.5	11	13	15
Order No.	68011160	68011161	68011162	68011163	68011164

OmniTaper EV implant

Titanium¹, Titanium alloy², sterile

The DS OmniTaper implant is designed for replacing one or more missing teeth in order to restore chewing function.

- Endosseous section with OsseoSpeed surface
- Compatible with EV Prosthetics assortment
- Restoration: Various possibilities for type of fixation e.g., screw-, cement-, friction- and attachment-retained solutions. For one-position-only, six-position and non-indexed abutments
- Clinical use: one-stage or two-stage surgical procedures
- Premounted multifunctional TempBase that serves as a placement head, index impression and basis for temporary restorations
- Color coded
- Contains: Implant, Placement head (TempBase), Cover Screw
- Instruments needed: Implant Driver TempBase or optional Implant Driver EV

3. Cover Screw






Cover Screw EV

Titanium alloy², sterile

The Cover Screw is used for sealing the implant interface.

- Clinical use: two-stage surgical procedures
- Color coded

Cover Screw EV

					
	XS	S	M	L	XL
Order No.	68010001	68010002	68010005	68010006	68010007



4. TempBase Cap

TempBase Cap

Polypropylene³, non-sterile

The TempBase Cap is used for index registration during surgery and basis for temporary restorations.

TempBase Cap

			
	XS	S	M
		L	XL
Order No.	68010013	68010014	68010015

5. Healing abutments









HealDesign™ EV


Titanium alloy², sterile

The HealDesign EV is used for soft tissue sculpturing during the healing phase.


- Marked with diameter and height
- Clinical use: one-stage or two-stage surgical procedure
- Round shapes are indicated for all positions in the mouth
- Triangular shapes for anterior implant sites to mimic the incisors and canines
- Triangular HealDesign EV is a two-piece abutment
- Color coded

XS HealDesign EV

				
				
Ø mm	3.5	3.5	3.5	3.5
Height mm	2.5	3.5	4.5	6.5
Order No.	68013001	68013002	68013003	68013004

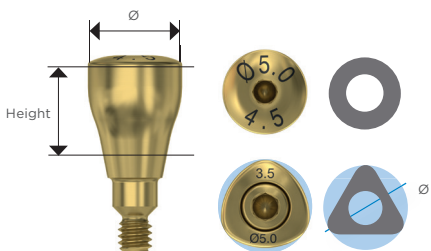

S HealDesign EV

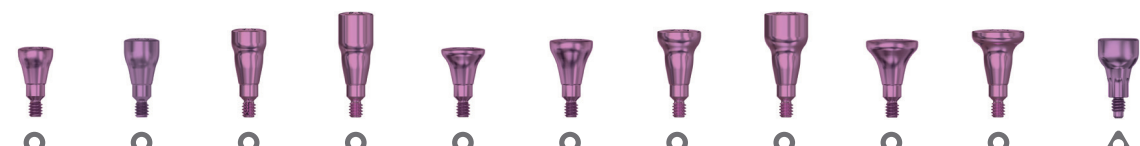


Ø mm	4	4	4	4	5	5	5	5	6	6	5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	4.5	3.5
Order No.	68013005	68013006	68013007	68013008	68013009	68013010	68013011	68013012	68013013	68013014	68013039

M HealDesign EV




Ø mm	5	5	5	5	6.5	6.5	6.5	6.5	5	6.5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	3.5
Order No.	68013015	68013016	68013017	68013018	68013019	68013020	68013021	68013022	68013040	68013041

L HealDesign EV



Ø mm	5	5	5	5	6.5	6.5	6.5	6.5	7.5	7.5	5	6.5
Height mm	2.5	3.5	4.5	6.5	2.5	3.5	4.5	6.5	3.5	4.5	3.5	3.5
Order No.	68013023	68013024	68013025	68013026	68013027	68013028	68013029	68013030	68013031	68013032	68013042	68013043

XL HealDesign EV



Ø mm	6.5	6.5	6.5	6.5	7.5	7.5
Height mm	2.5	3.5	4.5	6.5	3.5	4.5
Order No.	68013033	68013034	68013035	68013036	68013037	68013038


Healing abutments

Healing Abutment EV


Titanium alloy², sterile

The Healing Abutment EV is used for soft tissue sculpturing.

- Laser-etched bands for gauging
- Marked with diameter
- Color coded

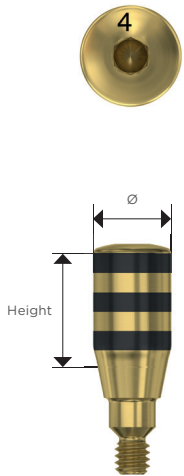

XS Healing Abutment EV

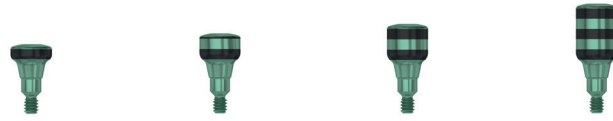

Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013044	68013045	68013046	68013047

S Healing Abutment EV



Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013048	68013049	68013050	68013051

M Healing Abutment EV



Ø mm	4	4	4	4
Height mm	2	3	4	6
Order No.	68013052	68013053	68013054	68013055

L Healing Abutment EV



Ø mm	4.3	4.3	4.3	4.3
Height mm	2	3	4	6
Order No.	68013056	68013057	68013058	68013059

XL Healing Abutment EV



Ø mm	4.8	4.8	4.8	4.8
Height mm	2	3	4	6
Order No.	68013060	68013061	68013062	68013063

6. Instruments

Guide Drill



Precision Drill



Order No.	68015133	68015134
-----------	----------	----------

All drills except the Precision Drill can be used for maximum ten cases. They should be carefully cleaned and sterilized after each surgery and replaced as soon as a decrease in their cutting efficiency is observed.

Initial drills

Guide Drill

Stainless steel¹, sterile

The Guide Drill is used for marking and to create a starting point.

- Multiple use

Precision Drill

Stainless steel¹, sterile

The Precision Drill is used for marking and to create a starting point.

- Single use

The Precision Drill is an extremely sharp drill and should be handled with caution to avoid injury.

OmniTaper Drill short



Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015098	68015099	68015100	68015101	68015102	68015103

Drills

OmniTaper Drill

Stainless steel¹, TiN-coated², sterile

The OmniTaper Drill is used for implant site preparation.


- Two-edged profile
- Multiple use
- Depth marked
- Color coded

OmniTaper Drill long



Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015086	68015087	68015088	68015089	68015090	68015091

Drill short 8-15mm
Drill long 8-18mm

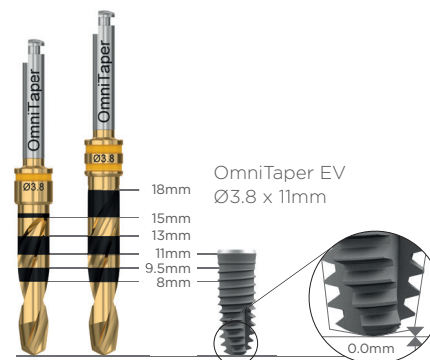

The effective drill depth matches the implant length.

OmniTaper Single Patient Drill

Stainless steel¹, ABS², sterile

The OmniTaper Single Patient Drill is used for implant site preparation.

- Single use
- Depth marked
- Color coded
- Available in short L 8-15mm

OmniTaper Single Patient Drill




Ø mm	2.0	3.0	3.4	3.8	4.5	5.5
Color coding						
Order No.	68015080	68015081	68015082	68015083	68015084	68015085

OmniTaper Crestal Drill

Stainless steel¹, TiN-coated³, sterile

The OmniTaper Crestal Drill is used for crestal implant site preparation according to the bone quality once the planned implant diameter has been reached.

- Multiple use
- Depth marked
- Color coded



OmniTaper Crestal Drill



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015092	68015093	68015094	68015095	68015096


Taps

OmniTaper Tap

Stainless steel¹, sterile

The OmniTaper Tap is used for additional tapping in cortical bone (D I).

- Multiple use
- Color coded
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

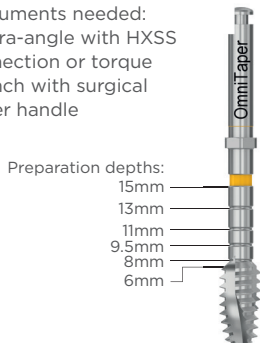

OmniTaper Tap



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015104	68015105	68015106	68015107	68015108

Implant Driver TempBase



Order No.	68015129	68015130
-----------	----------	----------

Implant Driver TempBase O-Ring



Order No.	68015131
-----------	----------

Implant Driver EV short



Ø mm	3.4	3.8	4.5	5.5
Color coding				
Order No.	68015188	68015190	68015192	68015194

Implant Driver EV long



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015187	68015189	68015191	68015193	68015195

Implant drivers

Implant Driver TempBase

Stainless steel¹, EPDM², non-sterile

The Implant Driver TempBase is used for installing OmniTaper implants with the TempBase (standard procedure).

- Dimple to facilitate correct positioning
- Applicable for all implant diameters
- Available in short/long
- Multiple use
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

Implant Driver TempBase O-Ring (spare part)

EPDM³, non-sterile

The Implant Driver TempBase O-Ring is used as spare part for Implant Driver TempBase.

- Multiple use

Implant Driver EV

Stainless steel¹, PEEK⁴, non-sterile

The Implant Driver EV is used for installing the implant without using the TempBase EV.

- Multiple use
- Depth marked
- Color coded
- Instruments needed: contra-angle with HXSS connection or torque wrench with surgical driver handle

The Implant Driver EV is not the standard driver for OmniTaper implants.


Planning aids

OmniTaper Direction Indicator

Titanium², non-sterile

The OmniTaper Direction Indicator is used for visualizing the position and direction of the prepared osteotomy and for measuring the space between osteotomies.

- Multiple use

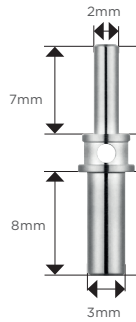

OmniTaper Direction Indicator




Order No.	68015097
-----------	----------

OmniTaper Try-In Implants

Titanium alloy², non-sterile

The OmniTaper Direction Indicator is used for intra-operative check of implant position, implant axis, congruency between implant and bone crest, and peri-implant soft tissue level.

- Design matches the DS OmniTaper implant
- Measure the thickness of the soft tissue
- Applicable for all implant lengths
- Multiple use
- Color coded



OmniTaper Try-In Implants



Ø mm	3.0	3.4	3.8	4.5	5.5
Color coding					
Order No.	68015237	68015238	68015239	68015240	68015241

Instrument Extender

Stainless steel³, non-sterile

The Instrument Extender is used for extending the length of a drill, a tap or the Implant Driver.

- Multiple use

Instrument Extender



Order No.	68015197
-----------	----------

OmniTaper Depth Gauge

Titanium alloy², non-sterile

The OmniTaper Depth Gauge is used for measuring the implant site before implant installation.


- Multiple use
- One end corresponds to the implant lengths
- One end is a measuring probe with 0-15 mm markings

OmniTaper Depth Gauge



Order No.	68015356
-----------	----------

OmniTaper Radiographic Template

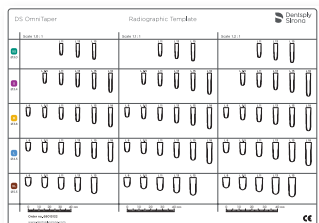

Order No. 68015132

OmniTaper Radiographic Template

PC[®], non-sterile

The OmniTaper Radiographic Template is a planning tool used prior to implant surgery.

- Used together with the X-ray of the patient's jaw
- Magnification range from 1.0 to 1.5 presented in two separate sheets

Torque Wrench EV



Order No. 25774

Torque Wrench

Torque Wrench EV

Stainless steel[†], non-sterile

The Torque Wrench is used together with the Surgical Driver Handle or the Restorative Driver Handle for tightening and measuring the torque.

- Used together with the Surgical Driver Handle for implant installation and adjustment
- Used together with the Restorative Driver Handle for tightening abutments and/or bridge screws
- Multiple use

Torque Wrench EV Surgical Driver Handle



Order No. 25775

Driver

Torque Wrench EV Surgical Driver Handle

Stainless steel[†], non-sterile

The Surgical Driver Handle is used together with the Torque Wrench.

- Multiple use

Torque Wrench EV Restorative Driver Handle



Order No. 25776 25777

Torque Wrench EV Restorative Driver Handle

Stainless steel[†], non-sterile

The Restorative Driver Handle is used together with the Torque Wrench.

- Multiple use

Hex Driver manual

Stainless steel¹, non-sterile

The Hex Driver manual is used for tightening screws, and surgical and restorative components.

Hex Driver manual



Total length mm	20	31
Order No.	25771	25772

Hex Driver

Stainless steel¹, non-sterile

The Hex Driver is used for tightening screws, and surgical and restorative components.

Hex Driver



Total length mm	20	24	35
Order No.	68015207	68015205	68015206

Surgical Trays

OmniTaper Surgical Tray

PPSU², silicone³ holders, non-sterile

The OmniTaper Surgical Tray is used during surgery and storage of OmniTaper surgical instruments.

- Instruments arranged in order of usage
- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments


Please contact customer service to order OmniTaper Surgical Kit (surgical tray and necessary instruments)

OmniTaper Surgical Tray




Size mm	Length 138	Width 190	Height 61.5
Order No.	68015282		

Upper tray

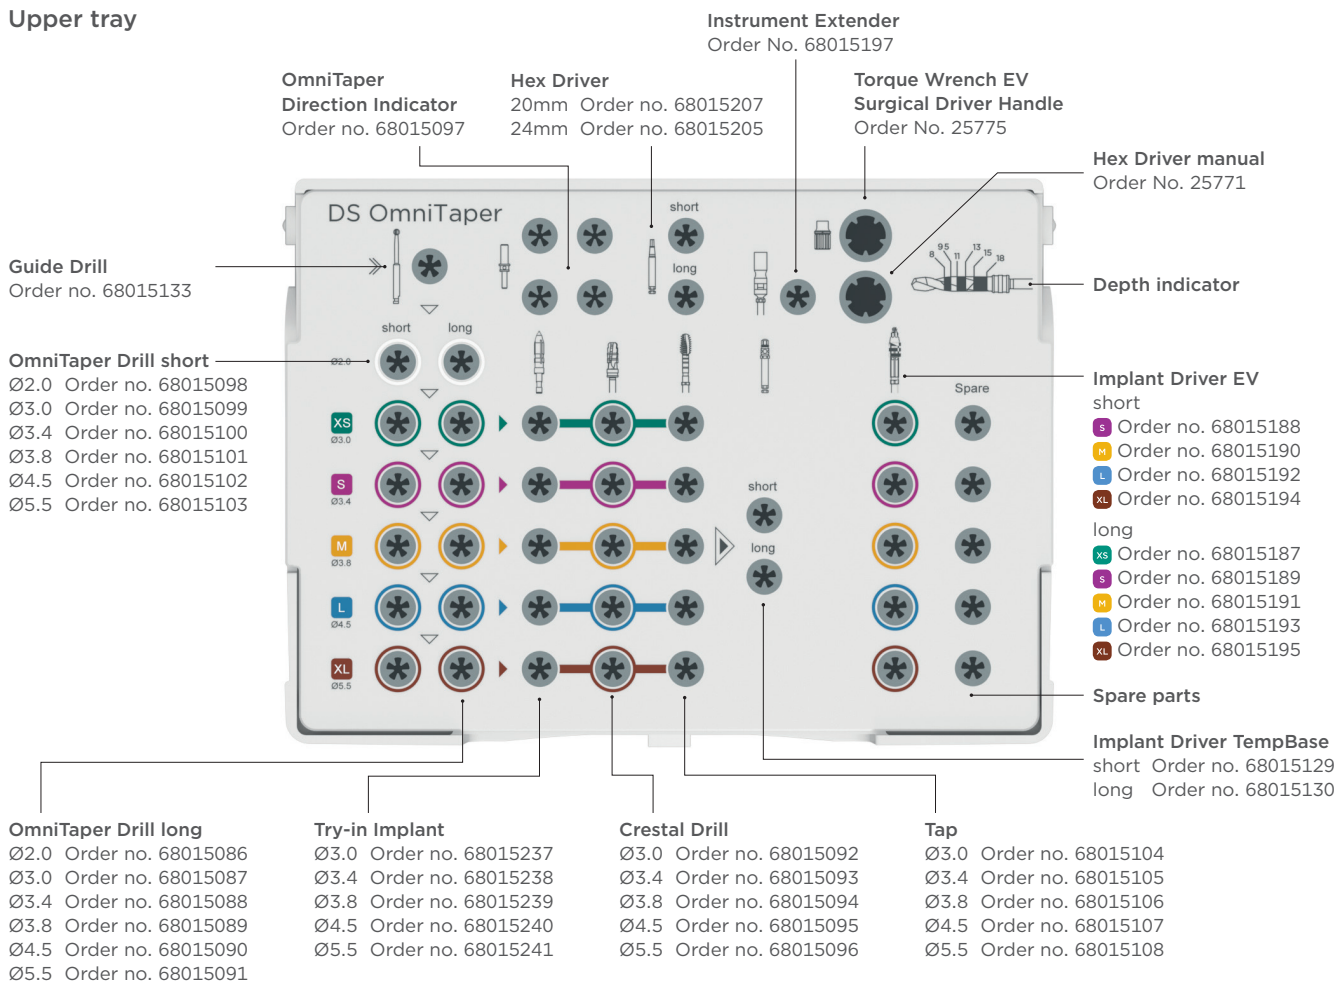

Lower tray

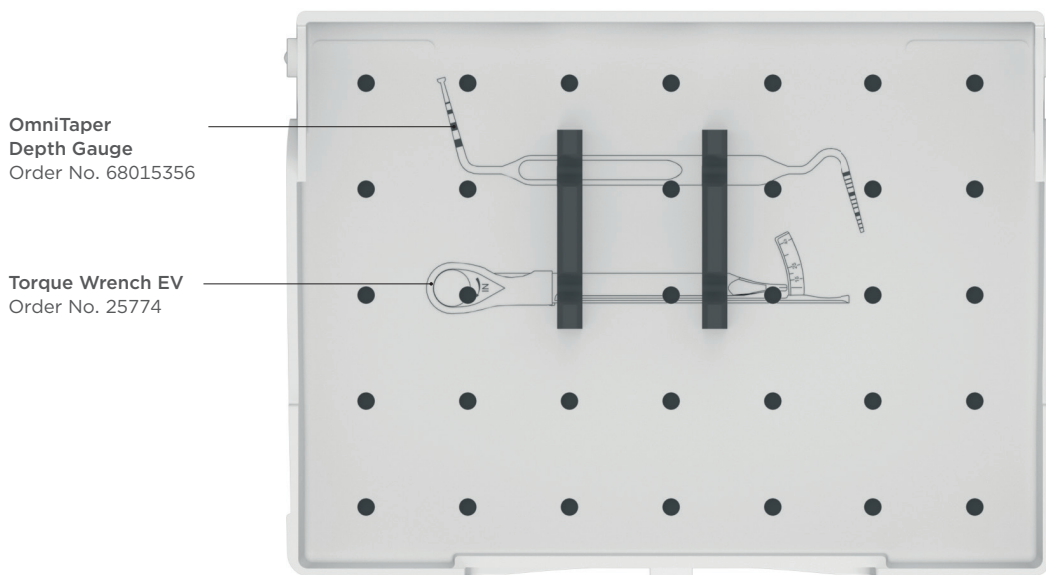

Washtray & Overlay


OmniTaper Washtray

Stainless steel¹, PEEK², silicon³, aluminum alloy⁴, non-sterile

The OmniTaper Washtray is used during surgery, for storage, machine cleaning, disinfection and subsequent steam sterilization of OmniTaper surgical instruments.

- Instrument fixation during vertical placement in washer-disinfector
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains: OmniTaper Washtray and removable OmniTaper Washtray Overlay

OmniTaper Washtray

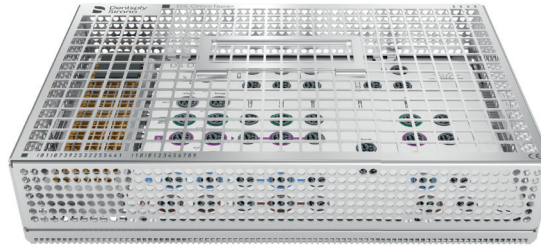

Size mm	Length 276	Width 176	Height 59
Order No.	68015271		

OmniTaper Washtray Overlay


Aluminum alloy⁵, non-sterile

The OmniTaper Washtray Overlay is used as a spare part for the OmniTaper Washtray.

- Colors and icons supporting surgical procedure

The overlay must be separated from the washtray before cleaning and re-assembled prior to sterilization. For further information, please refer to the Cleaning and sterilization instruction manual.

OmniTaper Washtray Overlay

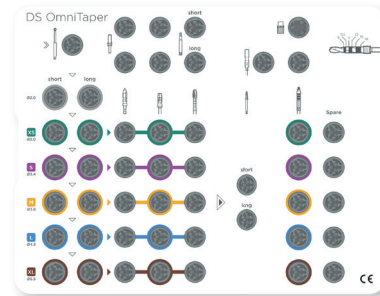

Order No.	68015272
-----------	----------

Washtray Sterilization Container



Order No. 68015266

Sterilization Container & Reusable Filter

Washtray Sterilization Container

Aluminum alloy¹, Stainless steel¹, PEEK², Silicone³, non-sterile

The Washtray Sterilization container is used for sterilization and storage of washtrays.

[The filter needs to be purchased separately](#)

Reusable Filter for Washtray Sterilization Container



Order No. 68015267

Reusable Filter for Washtray Sterilization Container

PTFE⁴, non-sterile

The Reusable Filter for Washtray Sterilization container is used as a spare part for Washtray Sterilization container.

- Multiple use
- Contains: 2 Reusable Filters for Washtray Sterilization Container

7. Guided Surgery Instruments

Specific instruments are available for guided implant installation of DS OmniTaper implants. These are marked "GS" (Guided Surgery) and can only be used together with the Simplant SAFE Guide and CEREC Guide 3.

When using Simplant software or Simplant planning service, case-specific guided surgery instruments can be ordered with the Simplant SAFE Guide.

Punch

OmniTaper Mucosal Punch GS

Stainless steel¹, sterile

The OmniTaper Mucosal Punch GS is used for minimally-invasive exposure of the surgical site.

- Single use
- Marked with diameter
- Color coded

OmniTaper Mucosal Punch GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017018	68017019	68017020	68017021

Drills

OmniTaper Initial Drill GS

Stainless steel¹, sterile

The OmniTaper Initial Drill GS is used for creating a starting point for the following drills and removal of soft tissue residue after use of the mucosa punch during guided surgery.

- Multiple use
- Marked with diameter
- Color coded

OmniTaper Initial Drill GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017111	68017119	68017127	68017135

OmniTaper Drill GS

Stainless steel¹, sterile

The OmniTaper Drill GS is used for implant site preparation up to the planned implant diameter.

- Multiple use
- Guided with the sleeve-on-drill system
- Marked with diameter
- Color coded

Drill Sleeve is needed and must be ordered separately

Drills, Crestal drill and Tap for guided surgery can only be used with the contra-angle handpiece.

OmniTaper Drill GS



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	8	8	8	8	8
Order No.	68017106	68017114	68017122	68017130	68017137

OmniTaper Drill GS



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	9.5	9.5	9.5	9.5	9.5
Order No.	68017110	68017118	68017126	68017134	68017141



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	11	11	11	11	11
Order No.	68017107	68017115	68017123	68017131	68017138



Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	13	13	13	13	13
Order No.	68017108	68017116	68017124	68017132	68017139

OmniTaper Drill GS




Ø mm	2.0	3.0	3.4	3.8	4.5
Color coding					
Length mm	15	15	15	15	15
Order No.	68017109	68017117	68017125	68017133	68017140

OmniTaper Crestal Drill GS

Stainless steel¹, sterile

The OmniTaper Crestal Drill GS is used for crestal implant site preparation according to the bone quality once the planned implant diameter has been reached.

- Multiple use
- Marked with diameter
- Depth marked
- Color coded



OmniTaper Crestal Drill GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017100	68017101	68017102	68017103


Taps

OmniTaper Tap GS

Stainless steel¹, sterile

The OmniTaper Tap GS is used for pre-tapping of the implant threads in cortical bone (D I).

- Multiple use
- Marked with diameter
- Depth marked (no mechanical depth stop)
- Color coded



OmniTaper Tap GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017014	68017015	68017016	68017017

OmniTaper Drill Sleeve GS narrow diameter



Ø mm	2.0	3.0	3.4	3.8
Order No.	68017105	68017113	68017121	68017129

OmniTaper Drill Sleeve GS wide diameter



Ø mm	2.0	3.0	3.4	3.8	4.5
Order No.	68017104	68017112	68017120	68017128	68017136

OmniTaper Implant Driver TempBase GS short



short	ND	WD
Order No.	68017034	68017035

OmniTaper Implant Driver TempBase GS long



long	ND	WD
Order No.	68017036	68017037

OmniTaper Sleeve for Implant Driver TempBase GS



Ø	ND	WD
Order No.	68017039	68017038

Sleeves

OmniTaper Drill Sleeve GS

Stainless steel[†], sterile

OmniTaper Drill Sleeve GS is used for safe guidance of the drills in the surgical guide.

- Single use
- Marked with ND (Narrow Diameter) for Ø3.0 – Ø3.8 implants or WD (Wide Diameter) for Ø4.5 implants

Must be used with the OmniTaper Drill GS

Driver

OmniTaper Implant Driver TempBase GS

Stainless steel[†], non-sterile

The OmniTaper Driver TempBase GS is used for installing OmniTaper implants with the TempBase using a contra-angle handpiece or the Torque Wrench.

- Markings on the shaft to align the abutment position and to monitor the rotational speed
- Marked with ND (Narrow Diameter) for implant Ø3.0 – Ø3.8 implants
- Marked with WD (Wide Diameter) for implant Ø4.5mm
- Sleeve is pre-mounted and can be replaced
- Torque: ≤ 50 Ncm
- Multiple use

Sleeves for Driver

OmniTaper Sleeve for Implant Driver TempBase GS

Stainless steel[†], non-sterile

The OmniTaper Sleeve for Implant Driver TempBase GS is used as a spare part for the OmniTaper Implant Driver TempBase.

- Multiple use
- Marked with ND (Narrow Diameter) or WD (Wide Diameter)

Stabilization Abutment

OmniTaper Stabilization Abutment GS

Titanium alloy², non-sterile

The stabilization abutment GS for TempBase prevents lateral movement of the surgical guide between the preparation of different implant sites and the second stabilization abutment GS. It also prevents the distortion of the guide.

- Multiple use
- Narrow diameter (ND) for Ø3.0 – Ø3.8 implants
- Wide diameter (WD) for Ø4.5 implants

OmniTaper Stabilization Abutment GS



Ø	ND	WD
Order No.	68017043	68017045

Positioning Aid

OmniTaper Positioning Aid EV GS

Titanium alloy², non-sterile

The OmniTaper Positioning Aid EV GS is used to secure implant analogs in the surgical guide in order to transfer the implant position, planned virtually, to a laboratory model (e.g. master cast, plaster cast).

- Multiple use

OmniTaper Positioning Aid EV GS



Ø mm	3.0	3.4	3.8	4.5
Color coding				
Order No.	68017040	68017041	68017042	68017044

Surgical Trays

OmniTaper Surgical Tray GS

PPSU⁷, silicone⁸ holders, non-sterile

The OmniTaper Surgical Tray GS is used during surgery and storage of OmniTaper surgical instruments.

- Two layers for instruments
- Grommet-less solution for easier cleaning
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains no instruments

Please contact customer service to order OmniTaper Surgical Kit GS (surgical tray and necessary instruments)

OmniTaper Surgical Tray GS



Size mm	Length 138	Width 190	Height 61.5
Order No.	68017203		

Upper tray

OmniTaper Drill GS

Ø2.0 x 8mm	Order no. 68017106	Ø3.0 x 8mm	Order no. 68017114	Ø3.4 x 8mm	Order no. 68017122	Ø3.8 x 8mm	Order no. 68017130
Ø2.0 x 9.5mm	Order no. 68017110	Ø3.0 x 9.5mm	Order no. 68017118	Ø3.4 x 9.5mm	Order no. 68017126	Ø3.8 x 9.5mm	Order no. 68017134
Ø2.0 x 11mm	Order no. 68017107	Ø3.0 x 11mm	Order no. 68017115	Ø3.4 x 11mm	Order no. 68017123	Ø3.8 x 11mm	Order no. 68017131
Ø2.0 x 13mm	Order no. 68017108	Ø3.0 x 13mm	Order no. 68017116	Ø3.4 x 13mm	Order no. 68017124	Ø3.8 x 13mm	Order no. 68017132
Ø2.0 x 15mm	Order no. 68017109	Ø3.0 x 15mm	Order no. 68017117	Ø3.4 x 15mm	Order no. 68017125	Ø3.8 x 15mm	Order no. 68017133

Ø4.5 x 8mm	Order no. 68017137
Ø4.5 x 9.5mm	Order no. 68017141
Ø4.5 x 11mm	Order no. 68017138
Ø4.5 x 13mm	Order no. 68017139
Ø4.5 x 15mm	Order no. 68017140


OmniTaper Initial Drill GS

Ø3.0	Order no. 68017111
Ø3.4	Order no. 68017119
Ø3.8	Order no. 68017127
Ø4.5	Order no. 68017135

OmniTaper Mucosal Punch GS

Ø3.0	Order no. 68017018
Ø3.4	Order no. 68017019
Ø3.8	Order no. 68017020
Ø4.5	Order no. 68017021

Torque Wrench EV Surgical Driver Handle
Order no. 25775

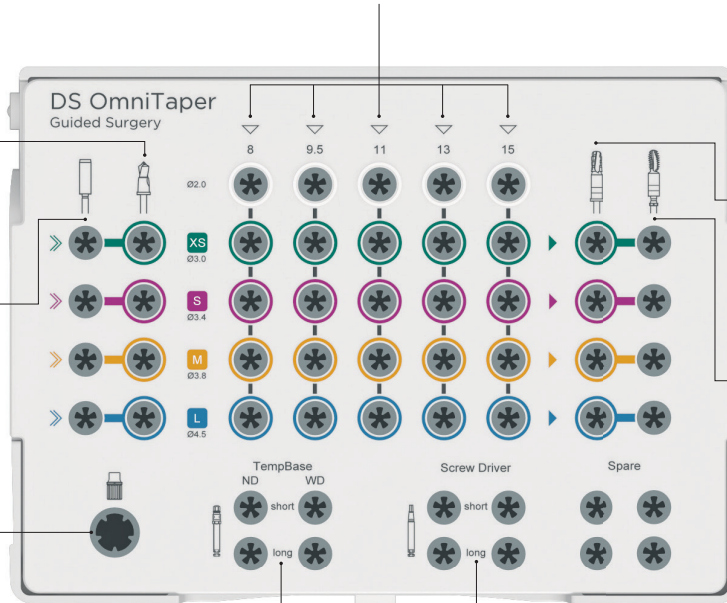

OmniTaper Crestal Drill GS

Ø3.0	Order no. 68017100
Ø3.4	Order no. 68017101
Ø3.8	Order no. 68017102
Ø4.5	Order no. 68017103

OmniTaper Tap GS

Ø3.0	Order no. 68017014
Ø3.4	Order no. 68017015
Ø3.8	Order no. 68017016
Ø4.5	Order no. 68017017

OmniTaper Implant Driver TempBase GS

ND short	Order no. 68017034
WD short	Order no. 68017035
ND long	Order no. 68017036
WD long	Order no. 68017037


Hex Driver

20mm	Order no. 68015207
24mm	Order no. 68015205

Lower tray

OmniTaper Depth Gauge
Order No. 68015356

Torque Wrench EV
Order No. 25774

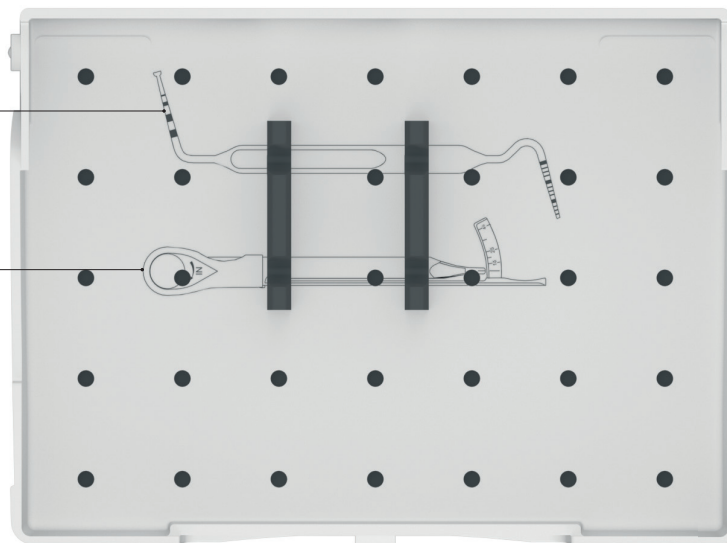


OmniTaper Washtray GS

Stainless steel¹, PEEK², silicon³, aluminum alloy², non-sterile

The OmniTaper Washtray GS is used during surgery and for storage, machine cleaning, disinfection and subsequent steam sterilization of OmniTaper surgical instruments.

- Instrument fixation during vertical placement in washer-disinfector
- Colors and icons supporting surgical procedure
- Scannable QR code for further information
- Contains: OmniTaper Washtray GS and removable OmniTaper Washtray GS Overlay

OmniTaper Washtray GS

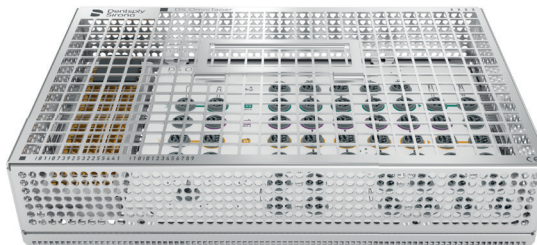

Size mm	Length 276	Width 176	Height 59
Order No.	68015354		

OmniTaper Washtray GS Overlay


Aluminum alloy², non-sterile

The OmniTaper Washtray GS Overlay is used as a spare part for the OmniTaper Washtray GS.

- Colors and icons supporting surgical procedure

The overlay must be separated from the washtray before cleaning and re-assembled prior to sterilization. For further information, please refer to the Cleaning and sterilization instruction manual.

OmniTaper Washtray GS Overlay

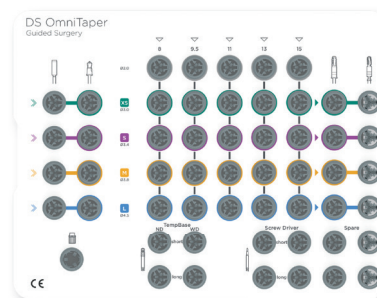

Order No.	68015355
-----------	----------

8. Material specifications

Index * will be found at material description for specific products.

Metals

Type	Index	Composition/Designation	Standard
Titanium	1	Ti grade 4	ASTM F67
Titanium alloy	2	Ti6Al4V ELI	ASTM F136
Stainless steel	3	Surgical stainless steel	ASTM F899
TiN Coating	4	Titanium Nitride	
Aluminum alloy	5	AlMg1	
Titanium	12	Ti grade 2	ASTM F67

Plastics

Type	Index	Composition/Designation	Standard
PEEK	6	Polyetheretherketone	
PPSU	7	Polyphenylsulfone	
Silicone	8	Polysiloxane	
ABS	9	Acrylonitrile butadiene styrene	
PC	10	Polycarbonate	
PP	11	Polypropylene	
EPDM	13	Ethylene propylene diene rubber	
PTFE	14	Polytetrafluoroethylene	

9. Index

By order number

Order No.	page	Order No.	page		
25771	Hex Driver 20mm manual.....	14	68013027	HealDesign EV (L) Ø6.5 2.5mm.....	7
25772	Hex Driver 31mm manual.....	14	68013028	HealDesign EV (L) Ø6.5 3.5mm.....	7
25774	Torque Wrench EV.....	13	68013029	HealDesign EV (L) Ø6.5 4.5mm.....	7
25775	Torque Wrench EV Surgical Driver Handle.....	13	68013030	HealDesign EV (L) Ø6.5 6.5mm.....	7
25776	Torque Wrench EV Rest. Driver Handle.....	13	68013031	HealDesign EV (L) Ø7.5 3.5mm.....	7
25777	Torque Wrench EV Rest. Driver Handle Low.....	13	68013032	HealDesign EV (L) Ø7.5 4.5mm.....	7
68010001	Cover Screw EV (XS).....	6	68013033	HealDesign EV (XL) Ø6.5 2.5mm.....	7
68010002	Cover Screw EV (S).....	6	68013034	HealDesign EV (XL) Ø6.5 3.5mm.....	7
68010005	Cover Screw EV (M).....	6	68013035	HealDesign EV (XL) Ø6.5 4.5mm.....	7
68010006	Cover Screw EV (L).....	6	68013036	HealDesign EV (XL) Ø6.5 6.5mm.....	7
68010007	Cover Screw EV (XL).....	6	68013037	HealDesign EV (XL) Ø7.5 3.5mm.....	7
68010013	TempBase Cap (XS)-(M).....	6	68013038	HealDesign EV (XL) Ø7.5 4.5mm.....	7
68010014	TempBase Cap (L).....	6	68013039	HealDesign EV (S) Ø5.0 3.5mm Triangular.....	7
68010015	TempBase Cap (XL).....	6	68013040	HealDesign EV (M) Ø5.0 3.5mm Triangular.....	7
68011140	OmniTaper EV Ø3.0 x 11mm.....	5	68013041	HealDesign EV (M) Ø6.5 3.5mm Triangular.....	7
68011141	OmniTaper EV Ø3.0 x 13mm.....	5	68013042	HealDesign EV (L) Ø5.0 3.5mm Triangular.....	7
68011142	OmniTaper EV Ø3.0 x 15mm.....	5	68013043	HealDesign EV (L) Ø6.5 3.5mm Triangular.....	7
68011143	OmniTaper EV Ø3.4 x 9.5mm.....	5	68013044	Healing Abutment EV (XS) 2mm.....	8
68011144	OmniTaper EV Ø3.4 x 11mm.....	5	68013045	Healing Abutment EV (XS) 3mm.....	8
68011145	OmniTaper EV Ø3.4 x 13mm.....	5	68013046	Healing Abutment EV (XS) 4mm.....	8
68011146	OmniTaper EV Ø3.4 x 15mm.....	5	68013047	Healing Abutment EV (XS) 6mm.....	8
68011147	OmniTaper EV Ø3.4 x 18mm.....	5	68013048	Healing Abutment EV (S) 2mm.....	8
68011148	OmniTaper EV Ø3.8 x 8mm.....	5	68013049	Healing Abutment EV (S) 3mm.....	8
68011149	OmniTaper EV Ø3.8 x 9.5mm.....	5	68013050	Healing Abutment EV (S) 4mm.....	8
68011150	OmniTaper EV Ø3.8 x 11mm.....	5	68013051	Healing Abutment EV (S) 6mm.....	8
68011151	OmniTaper EV Ø3.8 x 13mm.....	5	68013052	Healing Abutment EV (M) 2mm.....	8
68011152	OmniTaper EV Ø3.8 x 15mm.....	5	68013053	Healing Abutment EV (M) 3mm.....	8
68011153	OmniTaper EV Ø3.8 x 18mm.....	5	68013054	Healing Abutment EV (M) 4mm.....	8
68011154	OmniTaper EV Ø4.5 x 8mm.....	5	68013055	Healing Abutment EV (M) 6mm.....	8
68011155	OmniTaper EV Ø4.5 x 9.5mm.....	5	68013056	Healing Abutment EV (L) 2mm.....	8
68011156	OmniTaper EV Ø4.5 x 11mm.....	5	68013057	Healing Abutment EV (L) 3mm.....	8
68011157	OmniTaper EV Ø4.5 x 13mm.....	5	68013058	Healing Abutment EV (L) 4mm.....	8
68011158	OmniTaper EV Ø4.5 x 15mm.....	5	68013059	Healing Abutment EV (L) 6mm.....	8
68011159	OmniTaper EV Ø4.5 x 18mm.....	5	68013060	Healing Abutment EV (XL) 2mm.....	8
68011160	OmniTaper EV Ø5.5 x 8mm.....	5	68013061	Healing Abutment EV (XL) 3mm.....	8
68011161	OmniTaper EV Ø5.5 x 9.5mm.....	5	68013062	Healing Abutment EV (XL) 4mm.....	8
68011162	OmniTaper EV Ø5.5 x 11mm.....	5	68013063	Healing Abutment EV (XL) 6mm.....	8
68011163	OmniTaper EV Ø5.5 x 13mm.....	5	68015080	OmniTaper Drill SP Ø2.0 short.....	10
68011164	OmniTaper EV Ø5.5 x 15mm.....	5	68015081	OmniTaper Drill SP Ø3.0 short.....	10
68013001	HealDesign EV (XS) Ø3.5 2.5mm.....	6	68015082	OmniTaper Drill SP Ø3.4 short.....	10
68013002	HealDesign EV (XS) Ø3.5 3.5mm.....	6	68015083	OmniTaper Drill SP Ø3.8 short.....	10
68013003	HealDesign EV (XS) Ø3.5 4.5mm.....	6	68015084	OmniTaper Drill SP Ø4.5 short.....	10
68013004	HealDesign EV (XS) Ø3.5 6.5mm.....	6	68015085	OmniTaper Drill SP Ø5.5 short.....	10
68013005	HealDesign EV (S) Ø4.0 2.5mm.....	7	68015086	OmniTaper Drill Ø2.0 long.....	9
68013006	HealDesign EV (S) Ø4.0 3.5mm.....	7	68015087	OmniTaper Drill Ø3.0 long.....	9
68013007	HealDesign EV (S) Ø4.0 4.5mm.....	7	68015088	OmniTaper Drill Ø3.4 long.....	9
68013008	HealDesign EV (S) Ø4.0 6.5mm.....	7	68015089	OmniTaper Drill Ø3.8 long.....	9
68013009	HealDesign EV (S) Ø5.0 2.5mm.....	7	68015090	OmniTaper Drill Ø4.5 long.....	9
68013010	HealDesign EV (S) Ø5.0 3.5mm.....	7	68015091	OmniTaper Drill Ø5.5 long.....	9
68013011	HealDesign EV (S) Ø5.0 4.5mm.....	7	68015092	OmniTaper Crestal Drill Ø3.0.....	10
68013012	HealDesign EV (S) Ø5.0 6.5mm.....	7	68015093	OmniTaper Crestal Drill Ø3.4.....	10
68013013	HealDesign EV (S) Ø6.0 3.5mm.....	7	68015094	OmniTaper Crestal Drill Ø3.8.....	10
68013014	HealDesign EV (S) Ø6.0 4.5mm.....	7	68015095	OmniTaper Crestal Drill Ø4.5.....	10
68013015	HealDesign EV (M) Ø5.0 2.5mm.....	7	68015096	OmniTaper Crestal Drill Ø5.5.....	10
68013016	HealDesign EV (M) Ø5.0 3.5mm.....	7	68015097	OmniTaper Direction Indicator.....	12
68013017	HealDesign EV (M) Ø5.0 4.5mm.....	7	68015098	OmniTaper Drill Ø2.0 short.....	9
68013018	HealDesign EV (M) Ø5.0 6.5mm.....	7	68015099	OmniTaper Drill Ø3.0 short.....	9
68013019	HealDesign EV (M) Ø6.5 2.5mm.....	7	68015100	OmniTaper Drill Ø3.4 short.....	9
68013020	HealDesign EV (M) Ø6.5 3.5mm.....	7	68015101	OmniTaper Drill Ø3.8 short.....	9
68013021	HealDesign EV (M) Ø6.5 4.5mm.....	7	68015102	OmniTaper Drill Ø4.5 short.....	9
68013022	HealDesign EV (M) Ø6.5 6.5mm.....	7	68015103	OmniTaper Drill Ø5.5 short.....	9
68013023	HealDesign EV (L) Ø5.0 2.5mm.....	7	68015104	OmniTaper Tap Ø3.0.....	10
68013024	HealDesign EV (L) Ø5.0 3.5mm.....	7	68015105	OmniTaper Tap Ø3.4.....	10
68013025	HealDesign EV (L) Ø5.0 4.5mm.....	7	68015106	OmniTaper Tap Ø3.8.....	10
68013026	HealDesign EV (L) Ø5.0 6.5mm.....	7	68015107	OmniTaper Tap Ø4.5.....	10

Order No.		page	Order No.		page
68015108	OmniTaper Tap Ø5.5	10	68017041	OmniTaper Positioning Aid EV (S) GS	22
68015129	Implant Driver TempBase short	11	68017042	OmniTaper Positioning Aid EV (M) GS	22
68015130	Implant Driver TempBase long	11	68017043	OmniTaper Stabilization Abutment ND GS	22
68015131	Implant Driver TempBase O-Ring	11	68017044	OmniTaper Positioning Aid EV (L) GS	22
68015132	OmniTaper Radiographic Template	13	68017045	OmniTaper Stabilization Abutment WD GS	22
68015133	Guide Drill	9	68017100	OmniTaper Crestal Drill Ø3.0 GS	20
68015134	Precision Drill	9	68017101	OmniTaper Crestal Drill Ø3.4 GS	20
68015187	Implant Driver EV (XS) long	11	68017102	OmniTaper Crestal Drill Ø3.8 GS	20
68015188	Implant Driver EV (S) short	11	68017103	OmniTaper Crestal Drill Ø4.5 GS	20
68015189	Implant Driver EV (S) long	11	68017104	OmniTaper Drill Sleeve WD for Drill Ø2.0 GS	21
68015190	Implant Driver EV (M) short	11	68017105	OmniTaper Drill Sleeve ND for Drill Ø2.0 GS	21
68015191	Implant Driver EV (M) long	11	68017106	OmniTaper Drill Ø2.0 x 8mm GS	18
68015192	Implant Driver EV (L) short	11	68017107	OmniTaper Drill Ø2.0 x 11mm GS	19
68015193	Implant Driver EV (L) long	11	68017108	OmniTaper Drill Ø2.0 x 13mm GS	19
68015194	Implant Driver EV (XL) short	11	68017109	OmniTaper Drill Ø2.0 x 15mm GS	20
68015195	Implant Driver EV (XL) long	11	68017110	OmniTaper Drill Ø2.0 x 9.5mm GS	19
68015197	Instrument Extender	12	68017111	OmniTaper Initial Drill Ø3.0 GS	18
68015205	Hex Driver 24mm	14	68017112	OmniTaper Drill Sleeve WD for Drill Ø3.0 GS	21
68015206	Hex Driver 35mm	14	68017113	OmniTaper Drill Sleeve ND for Drill Ø3.0 GS	21
68015207	Hex Driver 20mm	14	68017114	OmniTaper Drill Ø3.0 x 8mm GS	18
68015237	OmniTaper Try-in Implant Ø3.0	12	68017115	OmniTaper Drill Ø3.0 x 11mm GS	19
68015238	OmniTaper Try-in Implant Ø3.4	12	68017116	OmniTaper Drill Ø3.0 x 13mm GS	19
68015239	OmniTaper Try-in Implant Ø3.8	12	68017117	OmniTaper Drill Ø3.0 x 15mm GS	20
68015240	OmniTaper Try-in Implant Ø4.5	12	68017118	OmniTaper Drill Ø3.0 x 9.5mm GS	19
68015241	OmniTaper Try-in Implant Ø5.5	12	68017119	OmniTaper Initial Drill Ø3.4 GS	18
68015266	Washtray Sterilization Container	17	68017120	OmniTaper Drill Sleeve WD for Drill Ø3.4 GS	21
68015267	Washtray Sterilization Container Filter 2x	17	68017121	OmniTaper Drill Sleeve ND for Drill Ø3.4 GS	21
68015271	OmniTaper Washtray	16	68017122	OmniTaper Drill Ø3.4 x 8mm GS	18
68015272	OmniTaper Washtray Overlay	16	68017123	OmniTaper Drill Ø3.4 x 11mm GS	19
68015282	OmniTaper Surgical Tray	14	68017124	OmniTaper Drill Ø3.4 x 13mm GS	19
68015354	OmniTaper Washtray GS	24	68017125	OmniTaper Drill Ø3.4 x 15mm GS	20
68015355	OmniTaper Washtray Overlay GS	24	68017126	OmniTaper Drill Ø3.4 x 9.5mm GS	19
68015356	OmniTaper Depth Gauge	12	68017127	OmniTaper Initial Drill Ø3.8 GS	18
68017014	OmniTaper Tap Ø3.0 GS	20	68017128	OmniTaper Drill Sleeve WD for Drill Ø3.8 GS	21
68017015	OmniTaper Tap Ø3.4 GS	20	68017129	OmniTaper Drill Sleeve ND for Drill Ø3.8 GS	21
68017016	OmniTaper Tap Ø3.8 GS	20	68017130	OmniTaper Drill Ø3.8 x 8mm GS	18
68017017	OmniTaper Tap Ø4.5 GS	20	68017131	OmniTaper Drill Ø3.8 x 11mm GS	19
68017018	OmniTaper Mucosal Punch Ø3.0 GS	18	68017132	OmniTaper Drill Ø3.8 x 13mm GS	19
68017019	OmniTaper Mucosal Punch Ø3.4 GS	18	68017133	OmniTaper Drill Ø3.8 x 15mm GS	20
68017020	OmniTaper Mucosal Punch Ø3.8 GS	18	68017134	OmniTaper Drill Ø3.8 x 9.5mm GS	19
68017021	OmniTaper Mucosal Punch Ø4.5 GS	18	68017135	OmniTaper Initial Drill Ø4.5 GS	18
68017034	OmniTaper Implant Driver TempBase ND short GS	21	68017136	OmniTaper Drill Sleeve WD for Drill Ø4.5 GS	21
68017035	OmniTaper Implant Driver TempBase WD short GS	21	68017137	OmniTaper Drill Ø4.5 x 8mm GS	18
68017036	OmniTaper Implant Driver TempBase ND long GS	21	68017138	OmniTaper Drill Ø4.5 x 11mm GS	19
68017037	OmniTaper Implant Driver TempBase WD long GS	21	68017139	OmniTaper Drill Ø4.5 x 13mm GS	19
68017038	OmniTaper Sleeve for Implant Driver TempBase WD GS	21	68017140	OmniTaper Drill Ø4.5 x 15mm GS	20
68017039	OmniTaper Sleeve for Implant Driver TempBase ND GS	21	68017141	OmniTaper Drill Ø4.5 x 9.5mm GS	19
68017040	OmniTaper Positioning Aid EV (XS) GS	22	68017203	OmniTaper Surgical Tray GS	22

Alphabetical order

Order No.	page	Order No.	page
68010006	6	68013044	8
68010005	6	68013045	8
68010002	6	68013046	8
68010007	6	68013047	8
68010001	6	68015207	14
68015133	9	25771	14
68013023	7	68015205	14
68013024	7	25772	14
68013042	7	68015206	14
68013025	7	68015193	11
68013026	7	68015192	11
68013027	7	68015191	11
68013028	7	68015190	11
68013043	7	68015189	11
68013029	7	68015188	11
68013030	7	68015195	11
68013031	7	68015194	11
68013032	7	68015187	11
68013015	7	68015130	11
68013016	7	68015131	11
68013040	7	68015129	11
68013017	7	68015197	12
68013018	7	68015092	10
68013019	7	68017100	20
68013020	7	68015093	10
68013041	7	68017101	20
68013021	7	68015094	10
68013022	7	68017102	20
68013005	7	68015095	10
68013006	7	68017103	20
68013007	7	68015096	10
68013008	7	68015356	12
68013009	7	68015097	12
68013010	7	68015086	9
68013039	7	68015098	9
68013011	7	68017106	18
68013012	7	68017110	19
68013013	7	68017107	19
68013014	7	68017108	19
68013033	7	68017109	20
68013034	7	68015087	9
68013035	7	68015099	9
68013036	7	68017114	18
68013037	7	68017118	19
68013038	7	68017115	19
68013001	6	68017116	19
68013002	6	68017117	20
68013003	6	68015088	9
68013004	6	68015100	9
68013056	8	68017122	18
68013057	8	68017126	19
68013058	8	68017123	19
68013059	8	68017124	19
68013052	8	68017125	20
68013053	8	68015089	9
68013054	8	68015101	9
68013055	8	68017130	18
68013048	8	68017134	19
68013049	8	68017131	19
68013050	8	68017132	19
68013051	8	68017133	20
68013060	8	68015090	9
68013061	8	68015102	9
68013062	8	68017137	18
68013063	8	68017141	19

Order No.	page	Order No.	page
68017138	19	68017035	21
68017139	19	68017111	18
68017140	20	68017119	18
68015091	9	68017127	18
68015103	9	68017135	18
68017105	21	68017018	18
68017113	21	68017019	18
68017121	21	68017020	18
68017129	21	68017021	18
68017104	21	68017044	22
68017112	21	68017042	22
68017120	21	68017041	22
68017128	21	68017040	22
68017136	21	68015132	13
68015080	10	68017039	21
68015081	10	68017038	21
68015082	10	68017043	22
68015083	10	68017045	22
68015084	10	68015282	14
68015085	10	68017203	22
68011140	5	68015104	10
68011141	5	68017014	20
68011142	5	68015105	10
68011143	5	68017015	20
68011144	5	68015106	10
68011145	5	68017016	20
68011146	5	68015107	10
68011147	5	68017017	20
68011148	5	68015108	10
68011149	5	68015237	12
68011150	5	68015238	12
68011151	5	68015239	12
68011152	5	68015240	12
68011153	5	68015241	12
68011154	5	68015271	16
68011155	5	68015354	24
68011156	5	68015272	16
68011157	5	68015355	24
68011158	5	68015134	9
68011159	5	68010014	6
68011160	5	68010015	6
68011161	5	68010013	6
68011162	5	25774	13
68011164	5	25776	13
68017036	21	25775	13
68017034	21	25777	13
68017037	21	68015266	17
		68015267	17



THE DENTAL
SOLUTIONS
COMPANY™

